


CASE STUDY

Avitus® Bone Harvester PSIS HARVEST

- No separate incision
- 9 minutes harvest time
- 15 CC's gold-standard cancellous bone
- 30 CC's gold-standard bone marrow captured
- Minimal blood loss
- Graft was used for a L4-S1 PLIF
- **Saved hospital \$1,200 in this case**

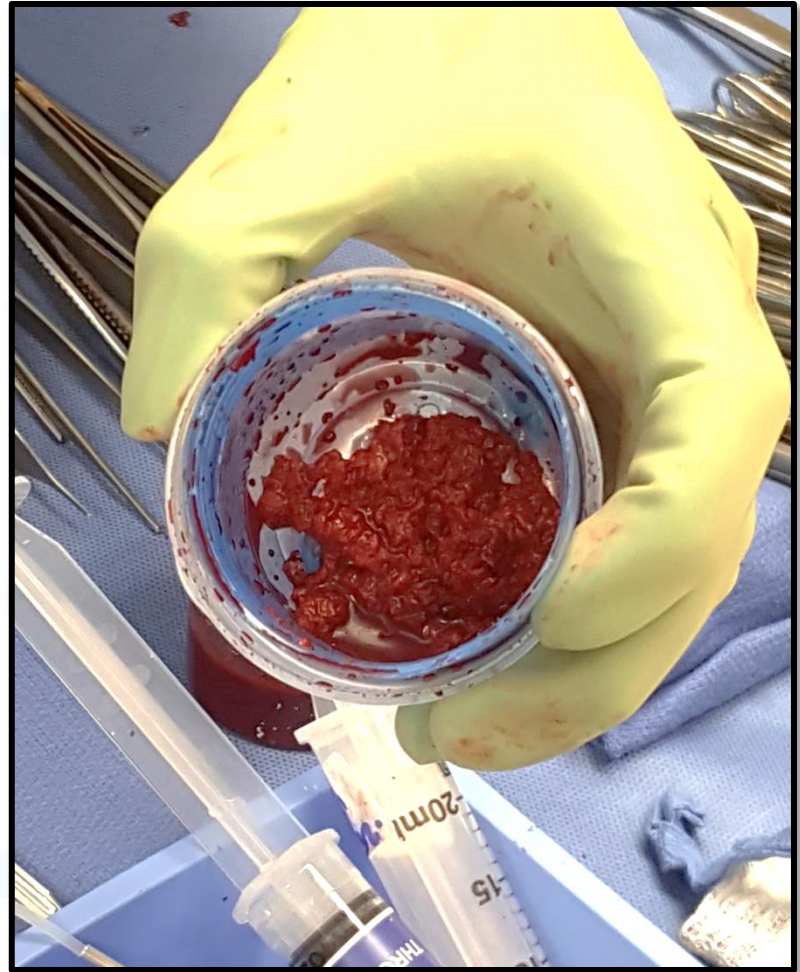

Shows Avitus® gold standard cancellous bone (marrow not shown)