


## Avitus® Bone Harvester PSIS HARVEST

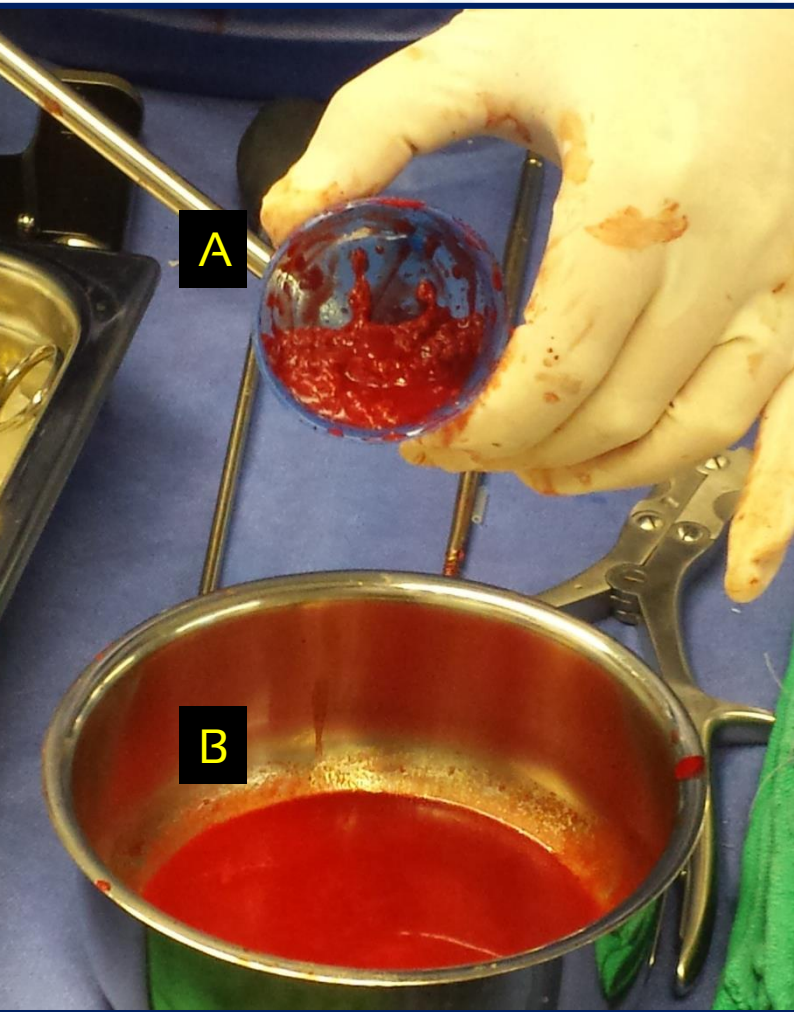

- 2cm minimally invasive incision
- 2.5 minutes harvest time
- 10 CC's gold-standard cancellous bone
- 30 CC's gold-standard bone marrow captured
- No blood loss from harvest
- Graft was used for a L4-L5 revision fusion

- A) Shows Avitus® gold standard Cancellous bone
- B) Shows Avitus® gold standard marrow