


Avitus® Bone Harvester DISTAL TIBIA HARVEST

- 3 minutes harvest time
- 10 CC's of gold-standard cancellous bone
- 5 CC's of gold-standard bone marrow captured
- Graft was successfully used for a Subtalar Joint revision fusion

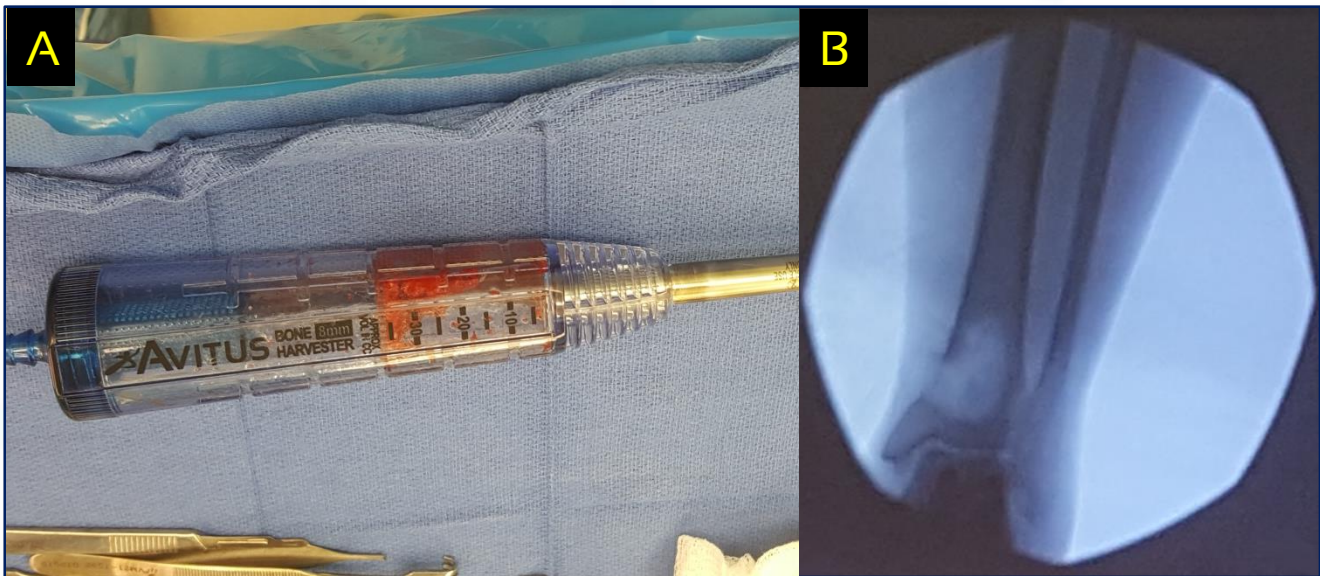

- A) Harvested graft material within Avitus® Bone Harvester
B) Radiograph of distal tibia harvest site